

इंटरनेट

मानक

Disclosure to Promote the Right To Information

Whereas the Parliament of India has set out to provide a practical regime of right to information for citizens to secure access to information under the control of public authorities, in order to promote transparency and accountability in the working of every public authority, and whereas the attached publication of the Bureau of Indian Standards is of particular interest to the public, particularly disadvantaged communities and those engaged in the pursuit of education and knowledge, the attached public safety standard is made available to promote the timely dissemination of this information in an accurate manner to the public.

“जानने का अधिकार, जीने का अधिकार”

Mazdoor Kisan Shakti Sangathan

“The Right to Information, The Right to Live”

“पुराने को छोड़ नये के तरफ”

Jawaharlal Nehru

“Step Out From the Old to the New”

IS 15441 (2004): Solid Mineral Fuels - Determination of Carbon and Hydrogen - Liebig Method [PCD 7: Solid Mineral Fuels]



“ज्ञान से एक नये भारत का निर्माण”

Satyanarayan Gangaram Pitroda

“Invent a New India Using Knowledge”



“ज्ञान एक ऐसा खजाना है जो कभी चुराया नहीं जा सकता है”

Bhartrhari—Nitiśatakam

“Knowledge is such a treasure which cannot be stolen”

BLANK PAGE



भारतीय मानक

ठोस खनिज ईंधन — कार्बन और हाइड्रोजन ज्ञात
करना — लाइबिग पद्धति

Indian Standard

SOLID MINERAL FUELS — DETERMINATION OF
CARBON AND HYDROGEN — LIEBIG METHOD

ICS 73.040

© BIS 2004

BUREAU OF INDIAN STANDARDS
MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG
NEW DELHI 110002

NATIONAL FOREWORD

This Indian Standard which is identical with ISO 625 : 1996 'Solid mineral fuels — Determination of carbon and hydrogen — Liebig method' issued by the International Organization for Standardization (ISO) was adopted by the Bureau of Indian Standards on the recommendations of the Solid Mineral Fuels Sectional Committee and approval of the Petroleum, Coal and Related Products Division Council.

The text of ISO Standard has been proposed to be approved as suitable for publication as an Indian Standard without deviations. Certain conventions are, however, not identical to those used in Indian Standards. Attention is particularly drawn to the following:

- a) Wherever the words 'International Standard' appear referring to this standard, they should be read as 'Indian Standard'.
- b) Comma (,) has been used as a decimal marker, while in Indian Standards, the current practice is to use a point (.) as the decimal marker.

Technical Corrigendum 1 to the above International Standard has been given at the end.

In this adopted standard reference appears to certain International Standards for which Indian Standards also exist. The corresponding Indian Standards which are to be substituted in their places are listed below along with their degree of equivalence for the editions indicated. However, that International Standard cross-referred in this adopted ISO Standard which has subsequently been revised, position in respect of latest ISO Standard has been given:

<i>International Standard</i>	<i>Corresponding Indian Standard</i>	<i>Degree of Equivalence</i>
ISO 331 : 1983 Coal — Determination of moisture in the analysis sample — Direct gravimetric method	IS 1350 (Part 1) : 1984 Methods of test for coal and coke: Part 1 Proximate analysis (<i>second revision</i>)	Technically not equivalent
ISO 687 : 1974 Coke — Determination of moisture in the analysis sample	IS 1350 (Part 1) : 1984 Methods of test for coal and coke: Part 1 Proximate analysis (<i>second revision</i>)	do
ISO 925 : 1997 Solid mineral fuels — Determination of carbonate carbon content — Gravimetric method	IS 1350 (Part 5) : 1979 Methods of test for coal and coke: Part 5 Special impurities (<i>first revision</i>) (Superseding IS 1352 : 1959)	do
ISO 1015 : 1992 Brown coals and lignites — Determination of moisture content — Direct volumetric method	IS 5062 (Part 1) : 2003 Methods of test for brown coal and lignites: Part 1 Determination of moisture content — Direct volumetric method (<i>first revision</i>)	Identical
ISO 1170 : 1977 Coal and coke — Calculation of analyses to different bases	Nil	—

(Continued on third cover)

Indian Standard

SOLID MINERAL FUELS — DETERMINATION OF CARBON AND HYDROGEN — LIEBIG METHOD

1 Scope

This International Standard specifies a method of determining the total carbon and the total hydrogen in hard coal, brown coal and lignite, and coke, by the Liebig method.

The results include the carbon in the carbonates and the hydrogen combined in the moisture and in the water of constitution of silicates. A determination of moisture is carried out at the same time, and an appropriate correction is applied to the hydrogen value obtained by combustion. A determination of carbon dioxide may also be made and the total carbon value corrected for the presence of mineral carbonates.

2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 331:1983, *Coal — Determination of moisture in the analysis sample — Direct gravimetric method.*

ISO 687:1974, *Coke — Determination of moisture in the analysis sample.*

ISO 925:1980, *Solid mineral fuels — Determination of carbon dioxide content — Gravimetric method.*

ISO 1015:1992, *Brown coals and lignites — Determination of moisture content — Direct volumetric method.*

ISO 1170:1977, *Coal and coke — Calculation of analyses to different bases.*

ISO 1988:1975, *Hard coal — Sampling.*

ISO 2309:1980, *Coke — Sampling.*

ISO 5068:1983, *Brown coals and lignites — Determination of moisture content — Indirect gravimetric method.*

ISO 5069-2:1983, *Brown coals and lignites — Principles of sampling — Part 2: Sample preparation for determination of moisture content and for general analysis.*

3 Principle

A known mass of coal or coke is burnt in a current of oxygen in a tube impervious to gases, the products of the incomplete combustion being further burnt over copper oxide; all the hydrogen is converted to water and all the carbon to carbon dioxide. These products are absorbed by suitable reagents and determined gravimetrically. Oxides of sulfur are retained by lead chromate, chlorine by a silver gauze roll and oxides of nitrogen by granular manganese dioxide.

4 Reagents and materials

WARNING — Care should be exercised when handling reagents, many of which are toxic.

During the analysis, unless otherwise stated, use only reagents of recognized analytical grade and only distilled water or water of equivalent purity.

4.1 Magnesium perchlorate, anhydrous, less than 1,2 mm in size and preferably within the size range 1,2 mm to 0,7 mm.

WARNING — Due regard must be taken of local regulations when disposing of exhausted magnesium perchlorate. Regeneration of magnesium perchlorate must not be attempted, owing to the risk of explosion.

4.2 Sodium hydroxide on an inert base, preferably of a coarse grading, for example 3,0 mm to 1,5 mm, but not finer than the grading 1,2 mm to 0,7 mm, and preferably of the self-indicating type.

4.3 Manganese dioxide, granular, 1,2 mm to 0,7 mm.

Manganese dioxide in the granular form and the size required can be prepared as follows.

Dissolve manganese sulfate in water and boil the solution. Make the solution alkaline with ammonium hydroxide and add solid ammonium persulfate, in small portions, to the boiling solution until precipitation is complete. Filter through a hardened fast-filter paper, wash with water by decantation, then with dilute sulfuric acid and finally with water until acid-free. Transfer the moist precipitate to a mortar and place in an oven until most of the water has evaporated, but the powder is still damp. Press the mass into a cake with a pestle, using firm pressure. Complete the drying, break up the cake cautiously and sieve to separate the 1,2 mm to 0,7 mm size.

4.4 Copper gauze, of mesh approximately 1 mm and 10 mm wide.

4.5 Copper oxide, wire form, chopped to particles approximately 3 mm long with a diameter of approximately 0,2 mm.

4.6 Lead chromate, fused, size range 2,4 mm to 1,2 mm.

4.7 Pure silver gauze, of mesh approximately 1 mm, made of wire approximately 0,3 mm in diameter.

4.8 Oxygen, hydrogen-free, preferably prepared from liquid air and not by electrolysis. Electrolytically prepared oxygen shall be passed over red-hot copper oxide before use to remove any trace of hydrogen.

4.9 Glass wool.

5 Apparatus

5.1 Analytical balance, capable of weighing to the nearest 0,1 mg.

5.2 Purification train, for absorbing water vapour and carbon dioxide from the oxygen used for the combustion. Assemble the train using a series of U-tubes containing the following reagents in the order stated, in the direction of flow:

- magnesium perchlorate (4.1) for absorbing water;
- sodium hydroxide on an inert base (4.2) for absorbing carbon dioxide;
- magnesium perchlorate for absorbing the water evolved in the reaction between carbon dioxide and sodium hydroxide.

The purification train shall be large enough to render frequent recharging unnecessary, even with continuous use.

5.3 Combustion assembly

5.3.1 Furnaces. The combustion tube is heated by three furnaces. For the 1,25 mm combustion tube described in clause 6, the following approximate lengths are appropriate:

- furnace No. 1 (to heat the boat and its contents to 925 °C) — 250 mm;
- furnace No. 2 (to keep the entire copper oxide section of the tube heated to 800 °C) — 500 mm;
- furnace No. 3 (to cover the lead chromate and the roll of pure silver gauze and to heat the former to about 500 °C) — 200 mm.

5.3.2 Combustion tube, of fused silica or suitable hard glass. The diameter of the tube shall be 12 mm to 15 mm. A suitable length is 1,25 m.

5.3.3 Combustion boat, of platinum, porcelain or fused silica, approximately 70 mm long.

5.4 Absorption train, for absorbing the water and carbon dioxide evolved by the combustion of the sample. Assemble the train using the following reagents in the order stated, in the direction of flow.

- magnesium perchlorate (4.1) for absorbing the water evolved during the combustion;

- b) granular manganese dioxide (4.3) for absorbing oxides of nitrogen;
- c) magnesium perchlorate for absorbing the water evolved from the manganese dioxide;
- d) sodium hydroxide on an inert base (4.2) for absorbing carbon dioxide;
- e) magnesium perchlorate for absorbing the water produced in the reaction between carbon dioxide and sodium hydroxide.

Midvale tubes (figure 1), which provide a large area of reaction, are used for all the reagents except

manganese dioxide, which is contained in a guard tube (figure 2), providing a long contact time with minimum mass.

A typical absorption train, with details of the packing, is shown in figure 3. A is the absorber for water, B is a guard-tube absorber for oxides of nitrogen, and C absorbs any water evolved from the manganese dioxide. Carbon dioxide is absorbed in D, the magnesium perchlorate in the upper portion absorbing any water produced in the reaction between carbon dioxide and sodium hydroxide. A second carbon dioxide absorber, E, should be added as a precautionary measure.

Dimensions in millimetres

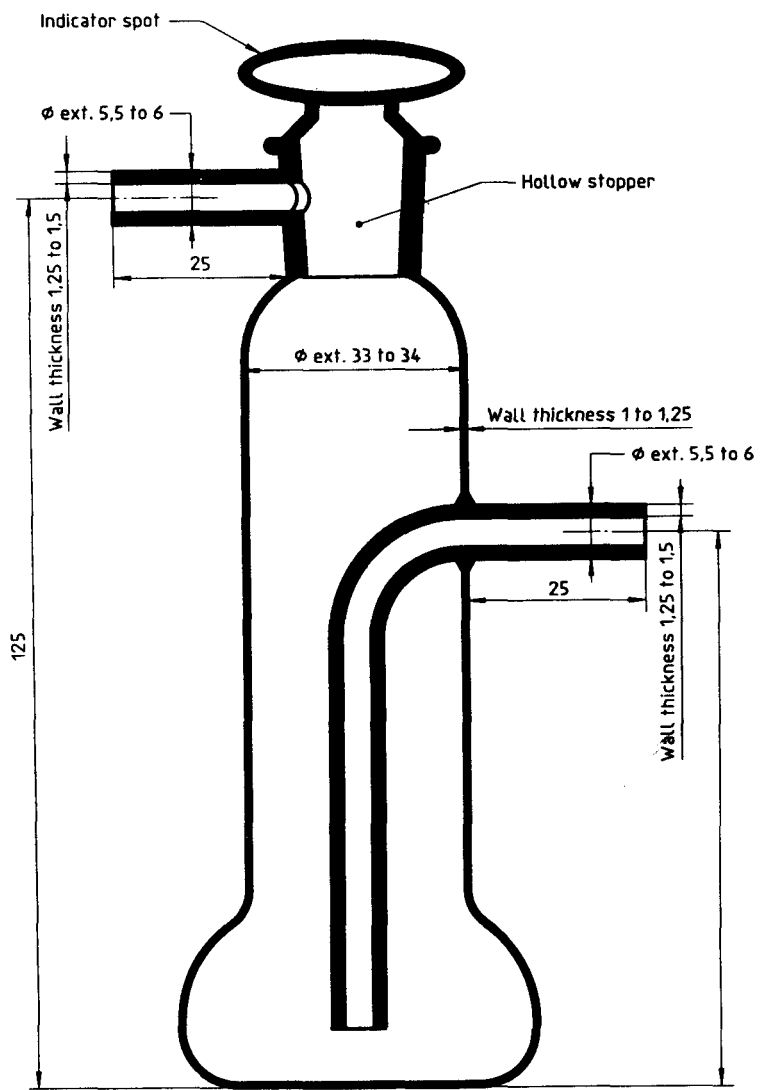


Figure 1 — Midvale tube

Dimensions in millimetres


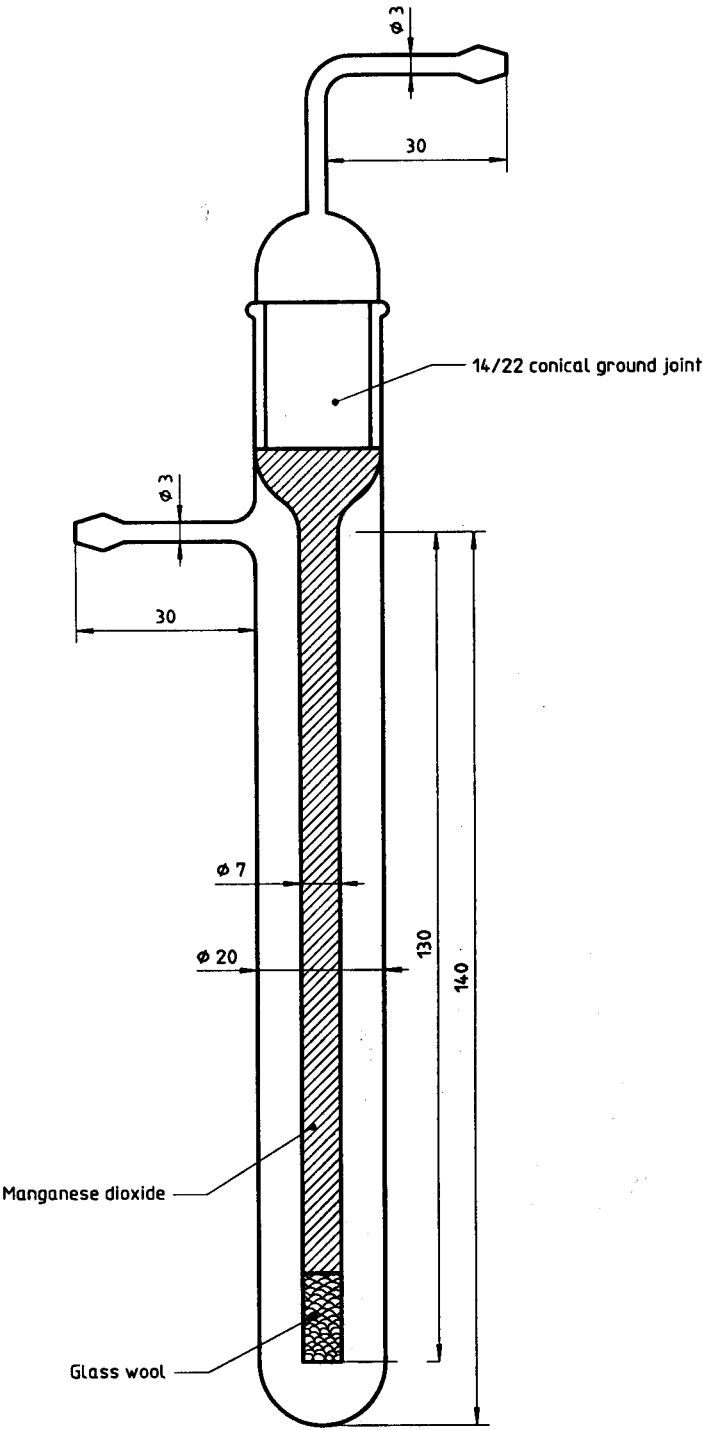


Figure 2 — Guard tube

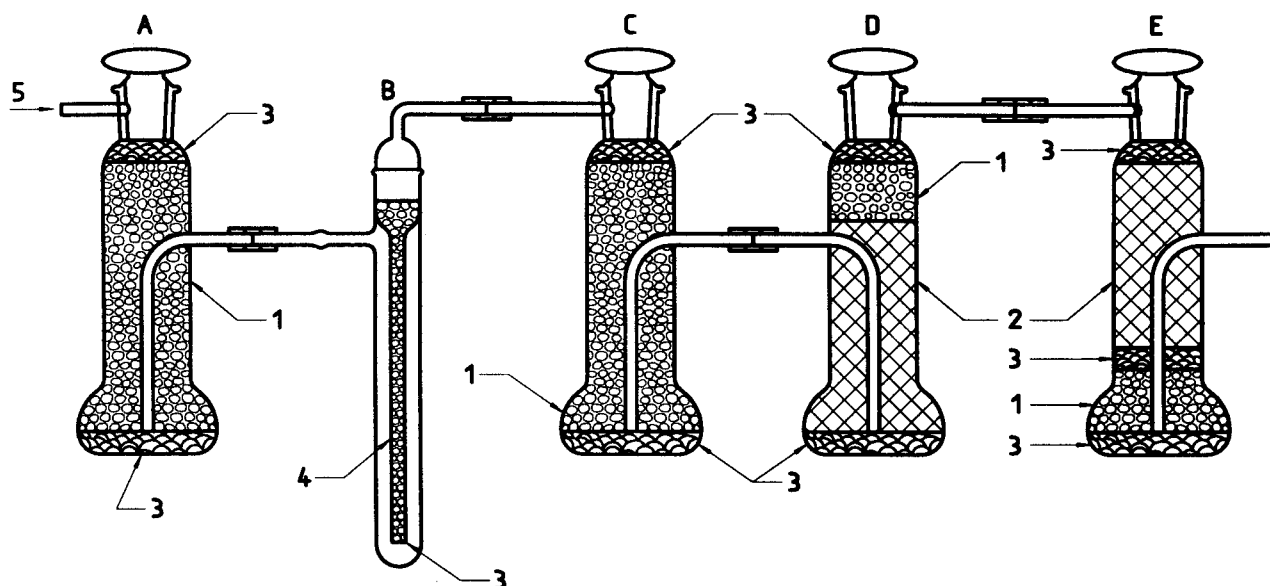

Key

- | | |
|---|---------------------|
| 1 Magnesium perchlorate, 1,2 mm to 0,7 mm size | 4 Manganese dioxide |
| 2 Sodium hydroxide (see 4.2), 1,2 mm to 0,7 mm size | 5 Inlet |
| 3 Glass wool | |

NOTE — In this illustration the optional second carbon dioxide absorber, E, is shown.

Figure 3 — Absorption train

Stoppered U-tubes may be used, if preferred, in place of the Midvale tubes.

Place glass wool (4.9), previously dried at 105 °C for 1 h, above and below the absorbents to prevent the carry-over of dust by the flow of oxygen, and to prevent the cracking of the Midvale tube by the heat of reaction.

If water is condensed in the first absorber, some nitrogen dioxide may dissolve in it and be considered as water. Because of the conversion factor from water to hydrogen, the error in the hydrogen determination thus caused is small, in the order of 0,05 % of hydrogen. This can only be avoided by heating the absorption tube to a temperature that is sufficiently high to prevent condensation of water.

NOTE 1 Oxides of nitrogen formed in the combustion would, in the absence of precautions, be absorbed by the sodium hydroxide and measured as carbon dioxide. The error in the carbon determination thus caused, in the order of 0,2 % of carbon, is substantially avoided by the use of a guard tube (see figure 2) in which the gases pass through an annular space to allow oxidation of nitrogen monoxide to

nitrogen dioxide which is absorbed by the manganese dioxide.

5.5 Oxygen flow-rate controller, a reducing valve on the oxygen cylinder together with a small needle valve and flowmeter, capable of measuring a flow of up to 100 ml/min, immediately before the purification train, is generally adequate. It may be useful to attach a bubbler device at the exit end of the assembled apparatus to give a visual indication of the rate of flow.

5.6 Heat-resistant stopper (acrylonitrile or chloroprene) for connecting the absorption train to the combustion tube.

5.7 Copper gauze roll, for constraining the reagents in the appropriate sections of the combustion tube (5.3.2). Roll the copper gauze into rolls 10 mm long and of sufficient diameter to ensure a close fit in the combustion tube.

5.8 Copper gauze spiral, through which passes a stout copper wire provided with a loop to facilitate removal from the combustion tube (5.3.2).

5.9 Silver gauze roll, for absorbing chlorine. Roll the pure silver gauze (4.7) to form a plug, 100 mm long and of sufficient diameter to ensure a close sliding fit in the combustion tube (5.3.2). A stout, pure silver wire is passed through the centre of the roll to facilitate its removal from the tube.

5.10 Heat-resistant wire, approximately 2,5 mm thick and 500 mm long, with a bent end to place the boat in the correct position in the combustion tube and to transfer the used boat from the combustion tube onto a rigid refractory sheet.

6 Preparation of the apparatus

6.1 Preparation of the combustion tube

For a combustion tube 1,25 m long and 12 mm to 15 mm in diameter, the following arrangement of the spacing is suitable:

- 10 mm space for a rubber stopper;
- 300 mm space to allow the furnace to be removed behind and away from the boat;
- 80 mm occupied by a copper gauze spiral (5.8) (see note 2);
- 70 mm space for the combustion boat (5.3.3);
- 50 mm space to prevent the front of the boat being heated too soon;
- 10 mm occupied by a plug roll of the copper gauze (5.7) (see note 2);
- 450 mm occupied by the copper oxide (4.5);
- 10 mm occupied by a plug roll of the copper gauze (see note 2);
- 100 mm occupied by the lead chromate (4.6);
- 10 mm occupied by a plug roll of the copper gauze;
- 100 mm occupied by a roll of the pure silver gauze (5.9);
- 50 mm space, with that section of tube wrapped on the outside with mineral fibre to prevent condensation of water inside;

— 10 mm space for a heat-resistant stopper (5.6).

The arrangement is shown in figure 4.

NOTE 2 The copper gauze spiral and rolls are oxidized during the preliminary heating in a current of oxygen.

6.2 Conditioning the combustion tube

Before starting a determination with a newly-packed combustion tube, heat the tube throughout its length, while passing a current of purified oxygen at a rate of 12 ml/min. Heating shall be continued for 3 h, with furnace No. 1 at a temperature of 925 °C, furnace No. 2 at a temperature of 800 °C and furnace No. 3, containing that portion of the tube packed with lead chromate and pure silver gauze, at a temperature of about 500 °C. The empty space adjacent to the exit end of the tube shall be heated in such a manner that, without charring the rubber stopper, condensation of steam is avoided.

6.3 Conditioning the absorption train

Connect the absorption train to the apparatus and purge with purified oxygen for 20 min, with the furnaces at their working temperatures. Disconnect absorbers A and D (and E, if used) (see figure 3) from the absorption train, seal the side-arms and close the taps, and allow them to cool to room temperature in a draught-free enclosure. Wipe each absorber with a clean lint-free cloth, remove the seals from the side-arms and weigh each absorber with a minimum of handling. Reconnect the absorption train to the combustion tube and reopen the taps. Particular care shall be taken to ensure that the inlet of the water-absorption tube of the absorption train is flush with the inner end of the rubber stopper in the combustion tube and that connections are made by bringing the ends of tubes close together, using the rubber tubing merely as a seal. After the absorption train has remained attached to the apparatus for a period of 2 h, remove and weigh absorbers A and D (and E, if used) as before, observing the same precautions as in the initial weighing. If each of these absorbers is within 0,000 5 g of its previous mass, the apparatus is considered to be in a proper condition for use.

NOTE 3 Under certain conditions of humidity, wiping the absorbers with a cloth may induce a static charge, which, if significant, could affect the weighing. The use of static eliminators should therefore be considered.

Dimensions in millimetres

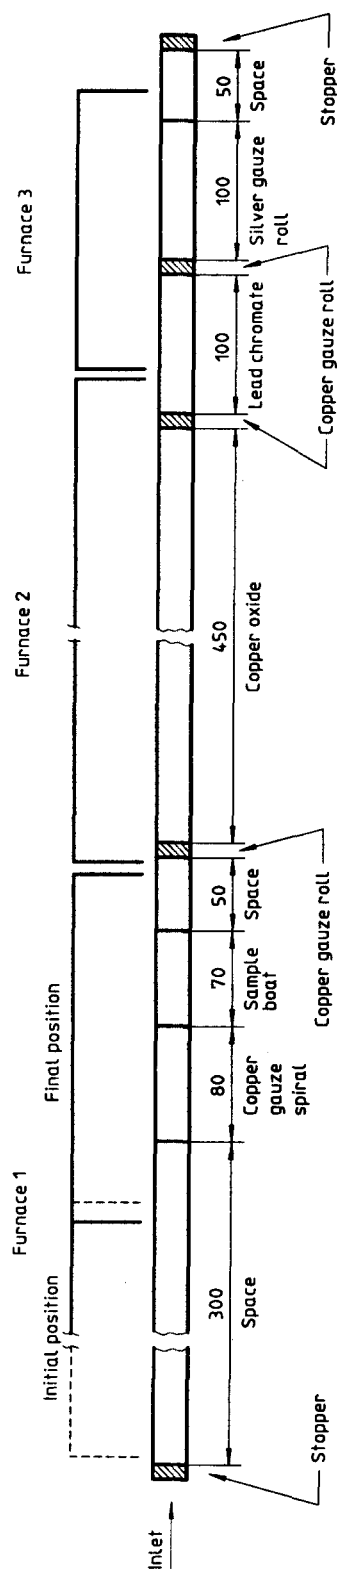


Figure 4 — Arrangement of the spacing in the combustion tube

7 Preparation of test sample

Prepare the test sample for general analysis in accordance with ISO 1988, ISO 2309 or ISO 5069-2, as appropriate. Ensure that the moisture content of the sample is in equilibrium with the laboratory atmosphere, exposing it, if necessary, in a thin layer for the minimum time to achieve equilibrium.

Before commencing the determination, thoroughly mix the test sample for at least 1 min, preferably by mechanical means.

After weighing the test portion (see clause 8), determine the moisture content using a further portion of the test sample by the method described in ISO 331, ISO 687, ISO 1015 or ISO 5068, as appropriate. A further portion should be set aside if the determination of carbon dioxide (ISO 925) is required.

8 Procedure

When starting the first determination of each day, raise the temperatures of the furnaces (5.3.1) to 925 °C, 800 °C and 500 °C respectively, while passing purified oxygen (4.8) through at a rate of 12 ml/min. Connect the absorption train (5.4) and purge for 20 min. Disconnect the train and weigh absorbers A, D and E, as described in 6.3. Switch off furnace No. 1 and allow it to cool.

Weigh accurately between 0,2 g and 0,3 g of the test sample, to the nearest 0,1 mg, and spread evenly over the bottom of a cool, previously ignited combustion boat (5.3.3). Connect the weighed absorption train to the combustion tube (5.3.2) as described in the previous paragraph. Place the combustion boat and the oxidized copper gauze spiral (5.8) in the combustion tube at the appropriate positions, insert the rubber stopper connecting the purification train and pass purified oxygen through the apparatus at a rate of 12 ml/min. Switch on furnace No. 1 and start the combustion by heating the copper gauze spiral. When the furnace is at 800 °C, gradually draw it forward to cover the combustion boat and its contents (see note 5), maintaining the passage of a steady stream of oxygen through the whole system while the sample is being burned. Continue until all visible carbon has disappeared (see note 4) and until the portion of the combustion tube containing the sample has been raised to 925 °C.

After combustion is complete, switch off furnace No. 1, allow the exit end of the combustion tube to cool and disconnect the absorption train. Wipe ab-

sorbers A, D and E, allow them to cool as described in 6.3 and weigh them (see note 7).

Carefully inspect the ash in the boat for unburnt carbon; if present, this invalidates the determination, which shall then be repeated.

Particular care must be taken during the combustion of brown coals and lignites, since heating too rapidly could result in incomplete combustion.

NOTES

4 Two hours are usually sufficient to complete the combustion of coal samples and 1 h may be sufficient for most coke samples.

5 Midvale tubes, used particularly for the absorption of carbon dioxide, cool slowly and up to 60 min should be allowed before weighing. When not connected to the apparatus, the Midvale tubes should be protected from atmospheric contamination by closing the taps and fitting guard seals of plugged rubber tubing to the open limbs. It is usual to weigh the absorption tubes without guard seals, after wiping.

9 Blank test

Carry out a blank test using the same procedure as described in clause 8, but omitting the test portion.

If the increase in mass of Midvale tube during the blank test is consistently greater than 0,001 g, the contents shall be discarded and the tube repacked. Furthermore, if at any time the increase in mass of tube E exceeds 0,05 g, the contents of tube D should be discarded and the tube repacked.

10 Expression of results

10.1 Total carbon content

The total carbon content, w_C , of the sample as analysed, expressed as a percentage by mass, is given by the equation

$$w_C = 27,29 \times \frac{m_2 - m_3}{m_1}$$

where

- m_1 is the mass, in grams, of the test portion;
- m_2 is the increase in mass, in grams, of absorbers B and C, determined in the test;
- m_3 is the increase in mass, in grams, of absorbers B and C, determined in the blank test (see clause 9).

10.2 Organic carbon content

The organic carbon content, $w_{C,o}$, of the sample as analysed (total carbon minus that present as carbonate in the mineral matter), expressed as a percentage by mass, is given by the equation

$$w_{C,o} = w_C - 0,272\ 9\ w_{CO_2}$$

where w_{CO_2} is the carbon dioxide content of the mineral carbonates in the sample as analysed (determined according to ISO 925), expressed as a percentage by mass.

10.3 Total hydrogen content

The total hydrogen content, w_H , of the sample as analysed, expressed as a percentage by mass, is given by the equation

$$w_H = 11,19 \times \frac{m_4 - m_5}{m_1}$$

where

- m_1 is the mass, in grams, of the test portion;
- m_4 is the increase in mass, in grams, of absorber A, determined in the test;
- m_5 is the increase in mass, in grams, of absorber A, determined in the blank test (see clause 9).

10.4 Total hydrogen content, less that present as moisture

The total hydrogen content, less that present as moisture, w_{H_1} (organic hydrogen plus that present in the water of constitution of the mineral matter), of the

sample as analysed, expressed as a percentage by mass, is given by the formula

$$w_{H_1} = w_H - 0,111\ 9M$$

where M is the moisture content, expressed as a percentage by mass, in the sample as analysed.

10.5 Additional information

The derivations of the factors used in the calculations in 10.1 to 10.4 are detailed in annex A.

Report the results as the mean of duplicate determinations, to the nearest 0,1 % (*m/m*) for the carbon determination and to the nearest 0,01 % (*m/m*) for the hydrogen determination.

The results of the determination described in this International Standard are reported on the "air-dried" basis. Calculation of results to other bases is dealt with in ISO 1170.

11 Precision

11.1 Repeatability limit

The results of duplicate determinations, carried out at different times, in the same laboratory, by the same operator with the same apparatus, on representative portions taken from the same analysis sample, should not differ by more than the values shown in table 1.

11.2 Reproducibility critical difference

The means of the results of duplicate determinations, carried out in each of two laboratories, on representative portions taken from the same sample after the last stage of sample preparation, should not differ by more than the values shown in table 1, at the 95 % confidence level.

Table 1

Element	Maximum acceptable difference between results (calculated for the same moisture content)	
	Repeatability limit	Reproducibility critical difference
Carbon	0,25 % absolute	0,5 % absolute
Hydrogen	0,12 % absolute	0,25 % absolute

12 Test report

The test report shall include the following information:

- a) the method used by reference to this International Standard;
- b) the identification of the sample tested;
- c) the results and the method of expression used;
- d) any unusual features noted during the determination;
- e) any operation not included in this International Standard, or regarded as optional;
- f) the date of the test:

Annex A (informative)

Derivation of factors used in calculations in clause 10

A.1 General

In this annex, relative atomic masses and relative molecular masses are represented by the chemical formulae in square brackets. The relative atomic masses given in table A.1 were used in the calculations.

Table A.1

Element	Symbol	Relative atomic mass
Carbon	C	12,011
Hydrogen	H	1,008
Oxygen	O	15,999

A.2 Carbon (see 10.1)

The total percentage of carbon, w_C , in the test sample is given by the formula

$$w_C = \frac{[C] \times (m_2 - m_3) \times 100}{[CO_2] \times m_1}$$

where

m_1 is the mass, in grams, of the test portion;

m_2 is the increase in mass, in grams, of absorbers B and C, determined in the test;

m_3 is the increase in mass, in grams, of absorbers B and C, determined in the blank test.

Hence

$$w_C = \frac{27,29 \times (m_2 - m_3)}{m_1}$$

A.3 Hydrogen (see 10.3)

The total percentage of hydrogen, w_H , in the test sample is given by the formula

$$w_H = \frac{[H_2] \times (m_4 - m_5) \times 100}{[H_2O] \times m_1}$$

where

m_1 is the mass, in grams, of the test portion;

m_4 is the increase in mass, in grams, of absorber A, determined in the test;

m_5 is the increase in mass, in grams, of absorber A, determined in the blank test.

Hence

$$w_H = \frac{11,19 \times (m_4 - m_5)}{m_1}$$

Solid mineral fuels — Determination of carbon and hydrogen — Liebig method

TECHNICAL CORRIGENDUM 1

Technical Corrigendum 1 to International Standard ISO 625:1996 was prepared by Technical Committee ISO/TC 27, *Solid mineral fuels*, Subcommittee SC 5, *Methods of analysis*.

Page 2, subclause 5.3.1

Change "1,25 mm" to "1,25 m" in line 2.

Page 6, subclause 6.1

Change "1,25 mm" to "1,25 m" in line 1.

Page 8, clause 8

Delete "(see note 5)" in lines 14 and 15 of the second paragraph.

Transfer the last paragraph before the notes to the second paragraph, before the final sentence.

Change "(see note 7)" to "(see note 5)" in the last line of the third paragraph.

Page 8, subclause 10.1

Change "B and C" to "D and E" in the fourth and sixth lines after the equation.

Page 11, clause A.2

Change "formula" to "equation" at the end of the first paragraph (introducing the equation).

Change "B and C" to "D and E" in the fourth and sixth lines after the equation.


Page 10, subclause 10.4

Page 11, clause A.3

Change "formula" to "equation" at the end of the first paragraph (introducing the equation).

Page 5, figure 3

Replace figure 3 by the following:

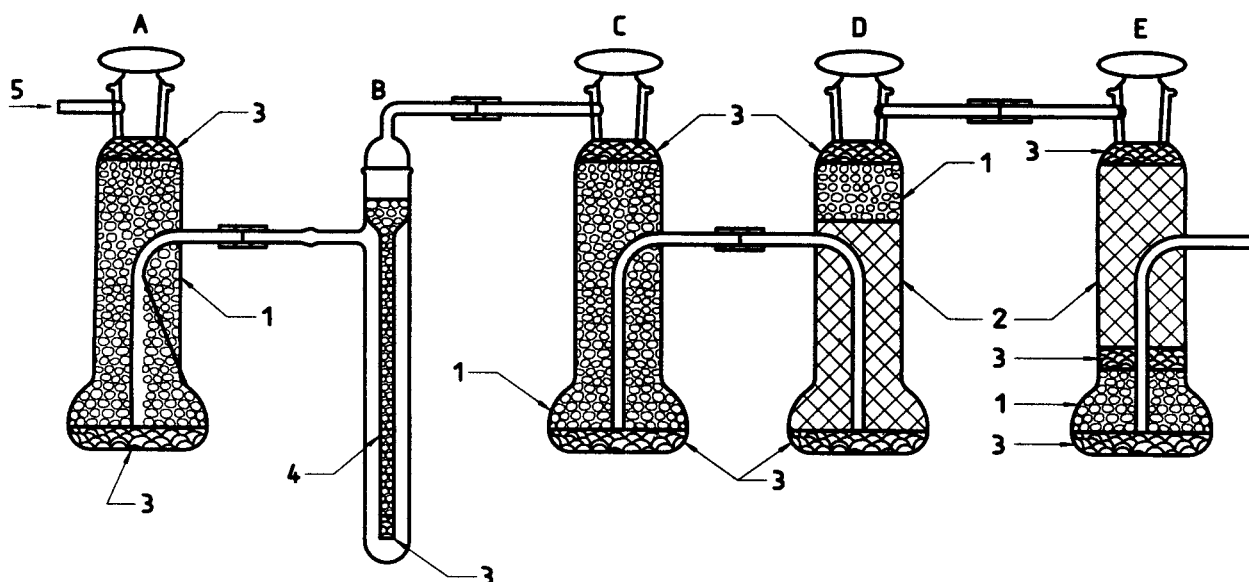

Key

- | | |
|--|---------------------|
| 1 Magnesium perchlorate, 1,2 mm to 0,7 mm size | 4 Manganese dioxide |
| 2 Sodium hydroxide (see 4.2) | 5 Inlet |
| 3 Glass wool | |

NOTE — In this illustration the optional second carbon dioxide absorber, E, is shown.

Figure 3 — Absorption train

(Continued from second cover)

<i>International Standard</i>	<i>Corresponding Indian Standard</i>	<i>Degree of Equivalence</i>
ISO 1988 : 1975 Hard coal — Sampling	IS 436 (Part 1/Sec 1) : 1964 Methods for sampling of coal and coke: Part 1 Sampling of coal, Section 1 Manual sampling (<i>revised</i>)	ISO 1988 and ISO 2309 cover both mechanical and manual sampling. These ISO Standards are being revised to cover manual sampling whereas mechanical sampling have been covered under ISO 13909 (Parts 1-8)
ISO 2309 : 1980 Coke — Sampling	IS 436 (Part 2) : 1965 Methods of sampling of coal and coke: Part 2 Sampling of coke	IS 436 (Part 1/Sec 1) and IS 436 (Part 2) are being revised to align with corresponding ISO Standards
ISO 5068 : 1983 Brown coals and lignites — Determination of moisture content — Indirect gravimetric method	Nil	—
ISO 5069-2 : 1983 Brown coals and lignites — Principles of sampling — Part 2 : Sample preparation for determination of moisture content and for general analysis	Nil	—

The Technical Committee responsible for the preparation of this standard will review the provisions of ISO 331, ISO 687, ISO 925, ISO 1015, ISO 1170, ISO 1988, ISO 2309, ISO 5068 and ISO 5069-2 and will decide whether they are acceptable for use in conjunction with this standard.

In reporting the results of a test or analysis, made in accordance with this standard, if the final value, observed or calculated, is to be rounded off, it shall be done in accordance with IS 2 : 1960 'Rules for rounding off numerical values (*revised*)'.

Bureau of Indian Standards

BIS is a statutory institution established under the *Bureau of Indian Standards Act, 1986* to promote harmonious development of the activities of standardization, marking and quality certification of goods and attending to connected matters in the country.

Copyright

BIS has the copyright of all its publications. No part of these publications may be reproduced in any form without the prior permission in writing of BIS. This does not preclude the free use, in the course of implementing the standard, of necessary details, such as symbols and sizes, type or grade designations. Enquiries relating to copyright be addressed to the Director (Publications), BIS.

Review of Indian Standards

Amendments are issued to standards as the need arises on the basis of comments. Standards are also reviewed periodically; a standard along with amendments is reaffirmed when such review indicates that no changes are needed; if the review indicates that changes are needed, it is taken up for revision. Users of Indian Standards should ascertain that they are in possession of the latest amendments or edition by referring to the latest issue of 'BIS Catalogue' and 'Standards: Monthly Additions'.

This Indian Standard has been developed from Doc : No. PCD 7 (1966).

Amendments Issued Since Publication

Amend No.	Date of Issue	Text Affected

BUREAU OF INDIAN STANDARDS

Headquarters :

Manak Bhavan, 9 Bahadur Shah Zafar Marg, New Delhi 110 002
Telephones : 2323 0131, 2323 33 75, 2323 9402

Telegrams : Manaksanstha
(Common to all offices)

Regional Offices :

	Telephone
Central : Manak Bhavan, 9 Bahadur Shah Zafar Marg NEW DELHI 110 002	{ 2323 7617 2323 3841
Eastern : 1/14 C.I.T. Scheme VII M, V. I. P. Road, Kankurgachi KOLKATA 700 054	{ 2337 8499, 2337 8561 2337 8626, 2337 9120
Northern : SCO 335-336, Sector 34-A, CHANDIGARH 160 022	{ 60 3843 60 9285
Southern : C.I.T. Campus, IV Cross Road, CHENNAI 600 113	{ 2254 1216, 2254 1442 2254 2519, 2254 2315
Western : Manakalaya, E9 MIDC, Marol, Andheri (East) MUMBAI 400 093	{ 2832 9295, 2832 7858 2832 7891, 2832 7892
Branches : AHMEDABAD. BANGALORE. BHOPAL. BHUBANESHWAR. COIMBATORE. FARIDABAD. GHAZIABAD. GUWAHATI. HYDERABAD. JAIPUR. KANPUR. LUCKNOW. NAGPUR. NALAGARH. PATNA. PUNE. RAJKOT. THIRUVANANTHAPURAM. VISAKHAPATNAM.	